

➤ Multi gas table | 0,5 l_n/min FLEXI-FLOW standard




* flow in l_n/min, range determined at 3 bar(a) inlet pressure and 1 bar(a) outlet pressure

** 10 bar max,

*** stated conversion uncertainty is on top of ±1,5% Rd plus ±0,5% FS accuracy of the instrument on N₂

➤ Multi gas table | 2 l_n/min FLEXI-FLOW standard

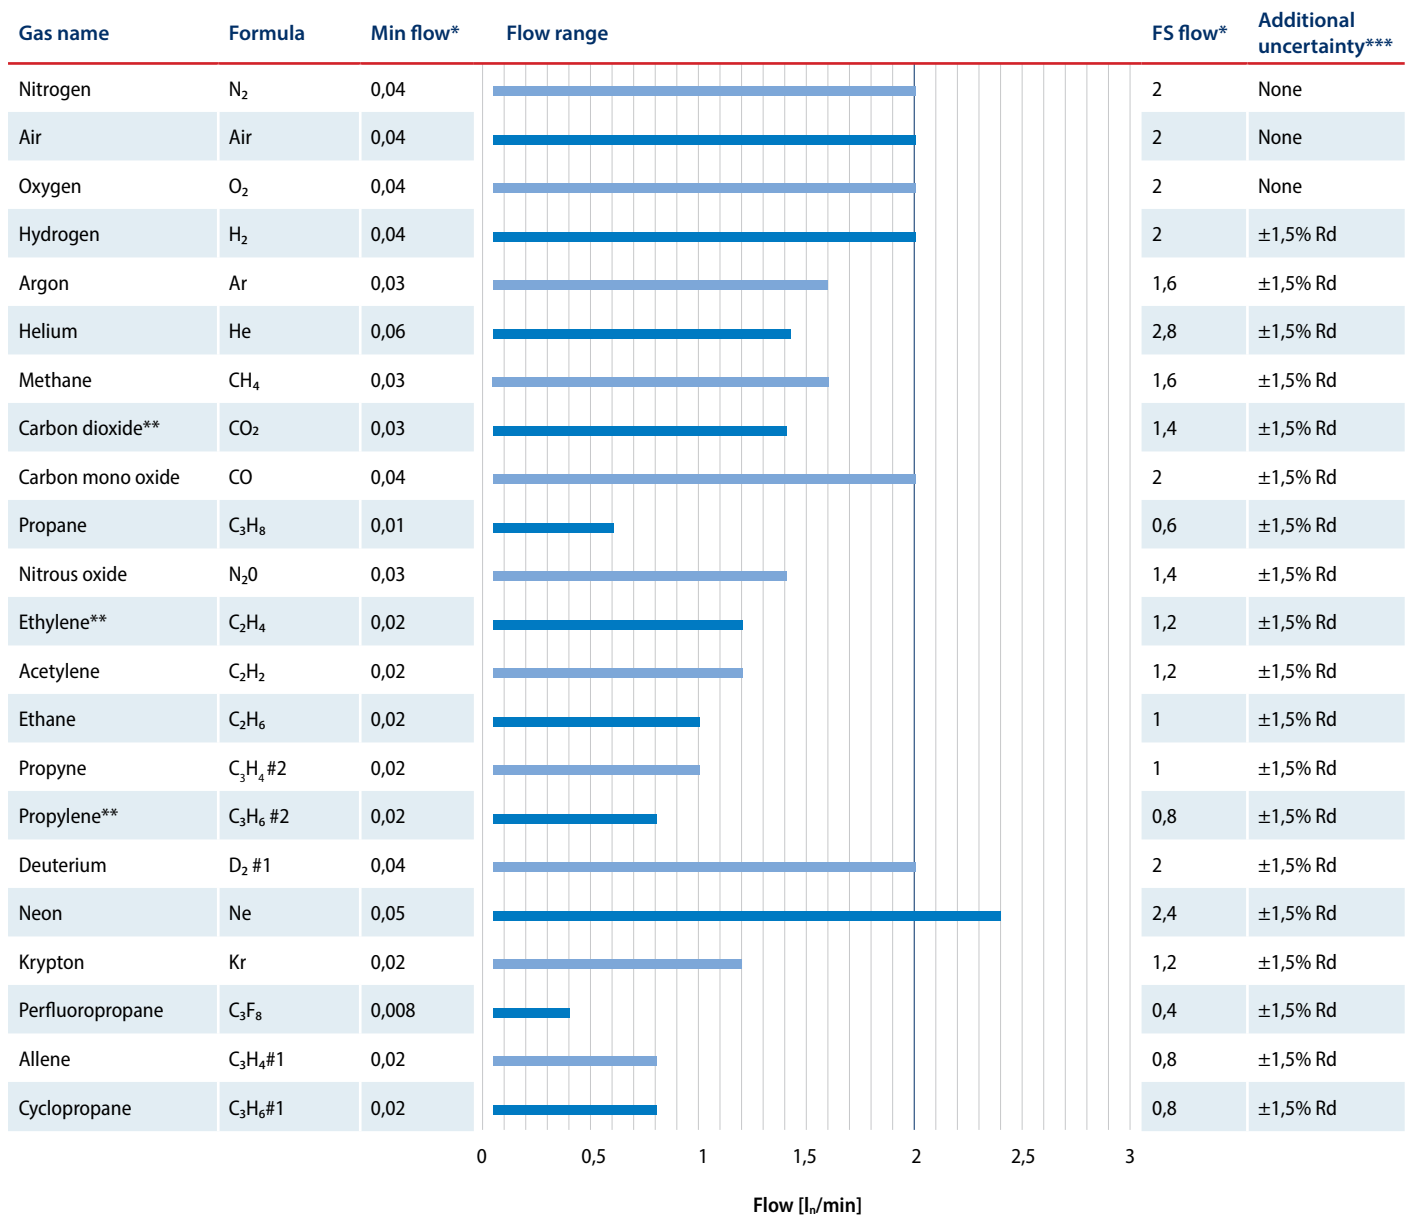


* flow in l_n/min, range determined at 3 bar(a) inlet pressure and 1 bar(a) outlet pressure

** 10 bar max,

*** stated conversion uncertainty is on top of ±1,5% Rd plus ±0,5% FS accuracy of the instrument on N₂

➤ Multi gas table | 5 l_n/min FLEXI-FLOW standard

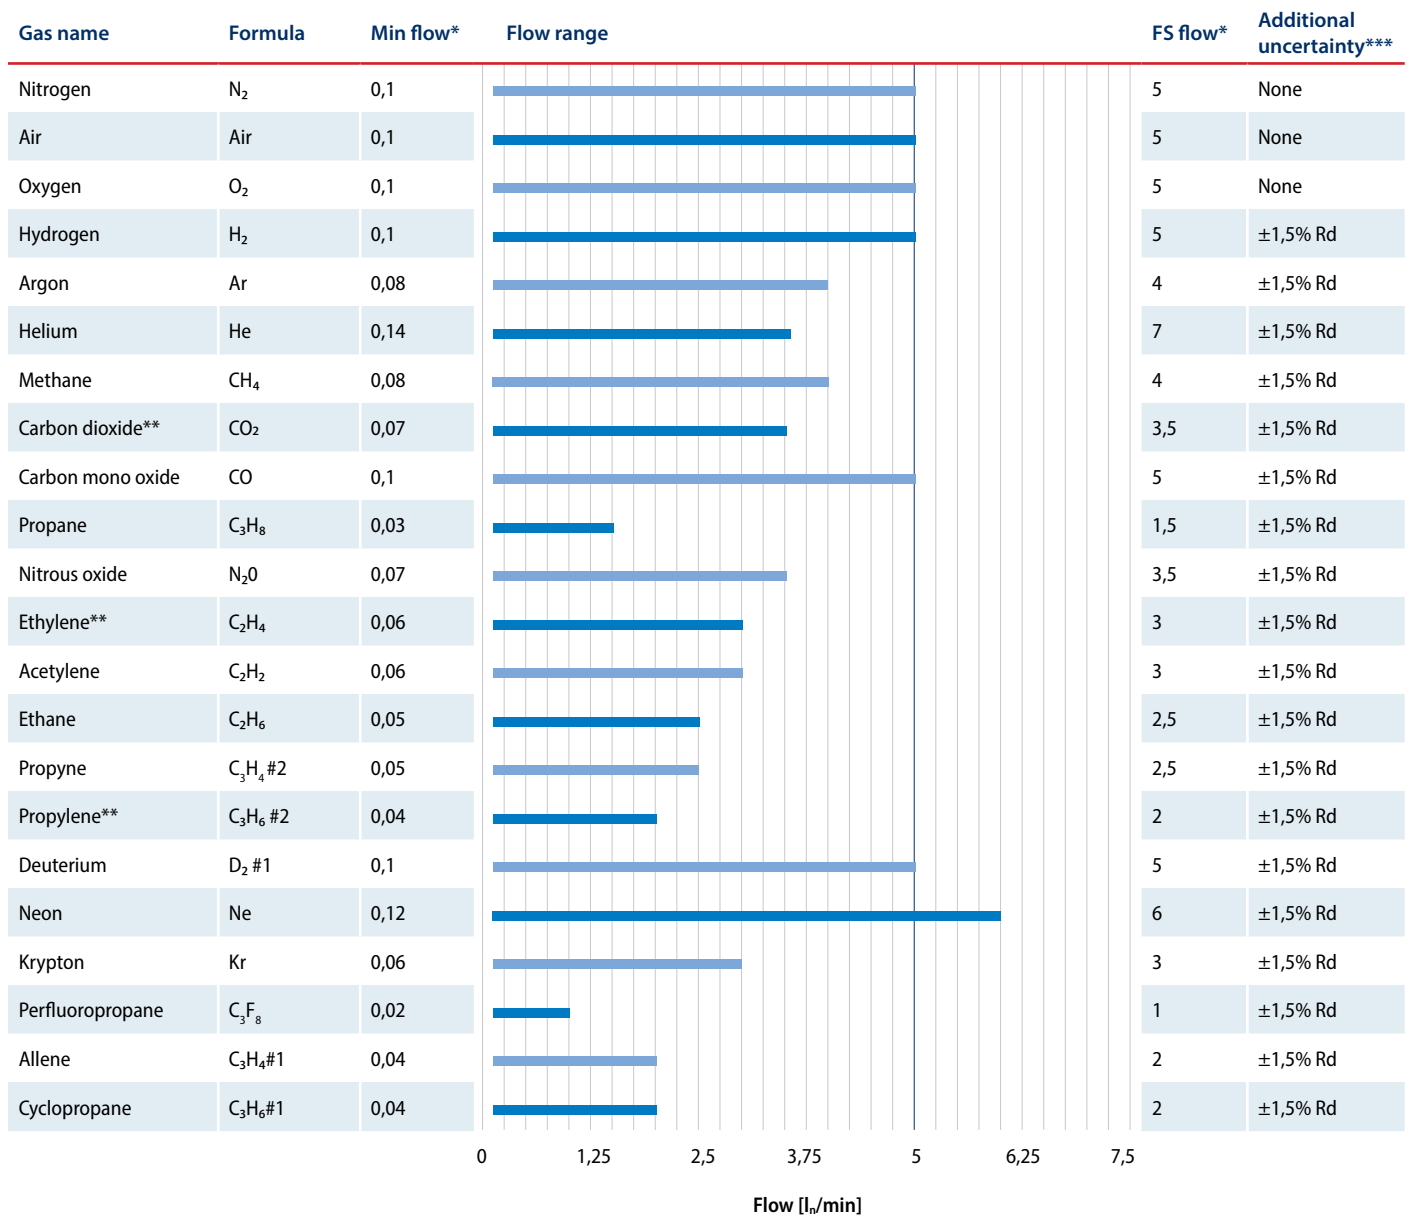


* flow in l_n/min, range determined at 3 bar(a) inlet pressure and 1 bar(a) outlet pressure

** 10 bar max,

*** stated conversion uncertainty is on top of ±1,5% Rd plus ±0,5% FS accuracy of the instrument on N₂

> Multi gas table | 20 l_n/min FLEXI-FLOW standard

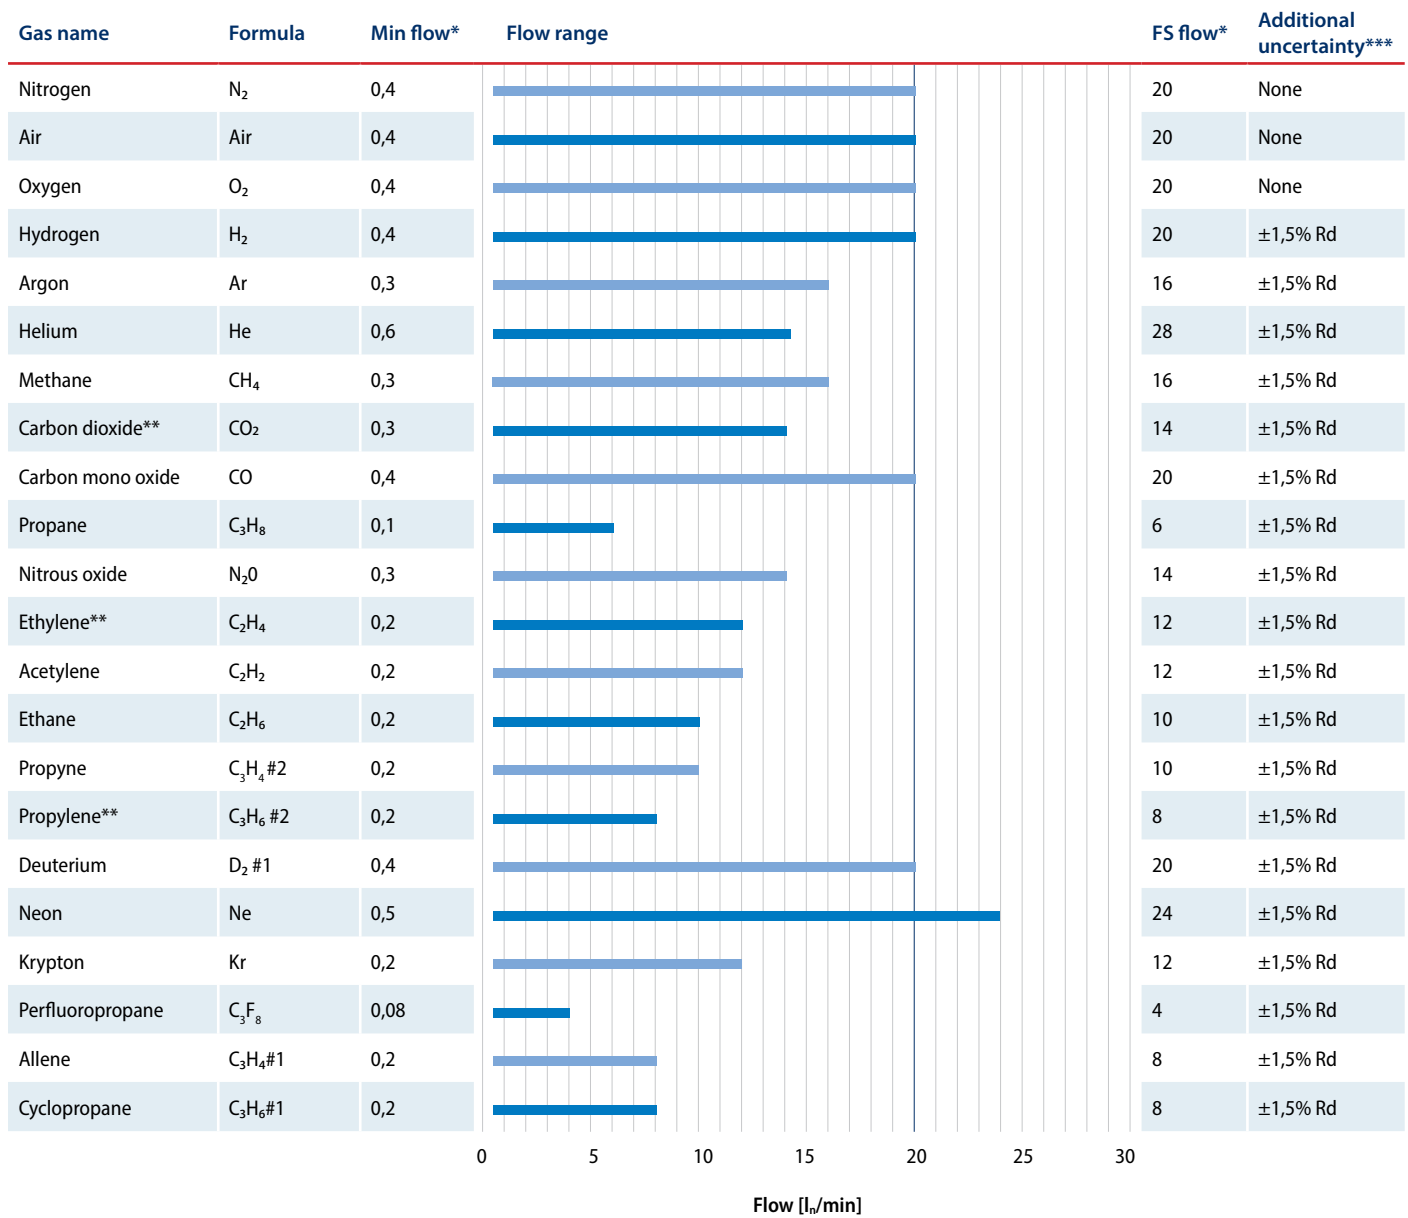

* flow in l_n/min, range determined at 3 bar(a) inlet pressure and 1 bar(a) outlet pressure

** 10 bar max,

*** stated conversion uncertainty is on top of ±1,5% Rd plus ±0,5% FS accuracy of the instrument on N₂